



Girton Cabinet Washer Model 072




- ♣ 316L Stainless steel construction with no interior threads.
- ♣ Rotating header spray system.
- ♣ Meets or exceeds ASME-BPE Standards.
- ♣ Single technical space.
- ♣ Fits through standard 36" door.
- ♣ All stainless steel dryer components.
- ♣ GAMP4 software design on controls
- ♣ 15 Ra header and spindles with no threads.
- ♣ 100% Borescope on all interior piping welds.
- ♣ Self-cleaning inline filter.

Phone: (570) 458-5521



Email: pharm1@girton.com

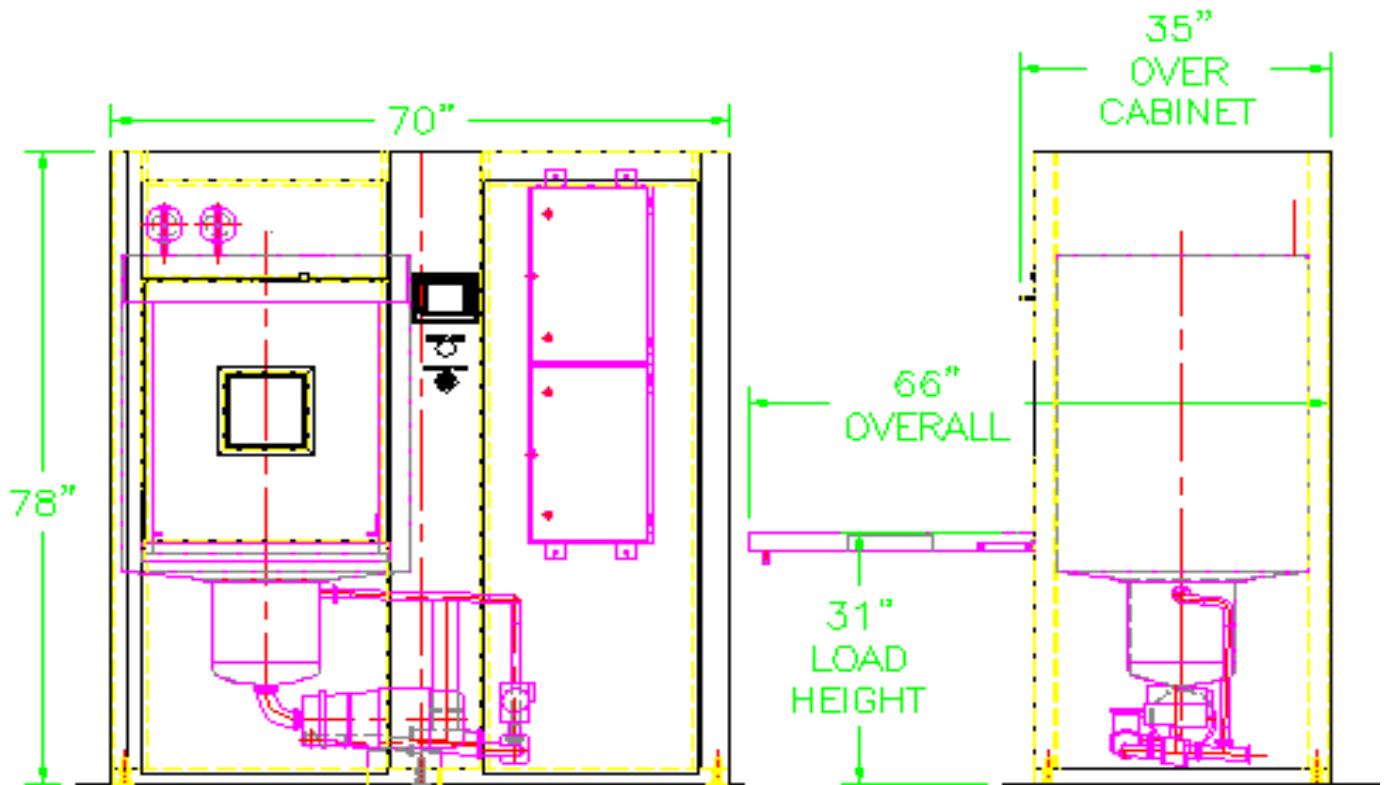

Description Specification Model 072:

- ♣ Left or Right Hand, Door to Service Side
- ♣ Single or Double Door Operation, the Self-Supporting Drop Down Door
- ♣ Steam or Electric Heating for Hot Water
- ♣ 2 Hp Recirculating Pump Delivering 60-Gallons Per Minute at 34' Head Pressure of Water
- ♣ Recirculation Header, Two Rotating Headers, Upper Header is Permanent in Washer, Lower Header is Part of Rack
- ♣ Allen Bradley MicroLogix ® PLC with Ethernet Communication with Panelview Plus 600 Touch Screen for Operator Control. A total of 16 programs can be stored in the PLC.
 - Password Protection for 4 Levels of Access to Control System
 - Alarm on Abnormal Condition - The washer has alarms based on each I/O point failure.
- ♣ Documentation, Validation requires documents evidence that the equipment or system will reliably perform in a manner consistent with the original design specifications.

Service Requirement:

- ♣ Electrical Heat: 3 Phase, 60 Cycle, 208/230/460 Volt
- ♣ Hot Water: 180°F Minimum Flow Rate 10 gpm at 35 psi, 16 Gallon Consumption/Cycle
- ♣ Purified Water: 180°F, 10 gpm at 30 psi, 3/4" Tri-Clamp Connection
- ♣ Steam: 60 psi at 50 Lbs./Hr. Recommended
- ♣ Condensate: 3/4" NPT
- ♣ Drain: 1 1/2" NPT From Machine to the Drain
- ♣ Ventilation: 4" Diameter Vent Collar, 50 CFM Minimum Removal Required
- ♣ Compressed Air: 1/4" NPT Connection, 90 psi Minimum, 1 CFM

GIRTON CABINET WASHER MODEL 072

1. DESCRIPTION

A Girton Model 072 Cabinet Washer is constructed of stainless steel and utilizes a rotating header spray system. The operating cycle is entirely automatic. A PLC controls each stage of the operation.

2. REGULATIONS, CODES AND STANDARDS

All engineering, design, manufacture and testing conforms to all applicable sections of the latest edition of the following codes, standards and specifications in effect at the time of order:

ASME-BPE - American Society of Mechanical Engineers

ANSI - American National Standard Institute

ASTM - American Society for Testing and Materials

OSHA - Occupation Safety and Health Administration

NEMA - National Electrical Manufacturers Associates

NEC - National Electrical Code

cGMP - Current Good Manufacturing Practices (CFR Title 21 parts 210 and 211)

NFPA - National Fire Protection Association

3. DIMENSIONS AND WEIGHT

- 3.1. Left Right Hand
- 3.2. Load Height: 31"
- 3.3. Overall Height: 78" Add 6" with dryer option
- 3.4. Overall Width: 70"
- 3.5. Overall Depth: 33 1/2"
- 3.6. Wash Chamber Size: 24" wide x 24" high x 24" deep
- 3.7. Operational Weight: _____ lbs.

4. CONSTRUCTION

4.1. Material Type and Finish:

- 4.1.1. **Washer Cabinet:** 14 gauge, T-304 T-316L stainless steel
Interior Finish: mill finish (2B) 35Ra or better 15Ra 8.5Ra
Exterior Finish: 35Ra or better
- 4.1.2. **Washer Tank:** 14 gauge, T-304 T-316L stainless steel
Interior Finish: mill finish (2B) 35Ra or better 15Ra 8.5Ra
Exterior Finish: 35Ra or better
- 4.1.3. **Insulation Jacket:** 20 gauge, T-304 stainless steel,
Exterior Finish: 35Ra or better
- 4.1.4. **Door:** T-304 T-316L stainless steel
Interior Finish: mill finish (2B) 35Ra or better 15Ra 8.5Ra
Exterior Finish: 35Ra or better
- 4.1.5. **Steam Heating Coil:** T-304 T-316L stainless steel
Electric Heat: Incolloy elements
- 4.1.6. **Steam and Condensate Piping:**
Interior on Washer: stainless steel T-304 T-316L schedule 10 pipe
Exterior on Washer: stainless steel T-304 schedule 40 pipe

- 4.1.7. **Compressed Air:**
 Tubing Poly-flo T-304 stainless steel.
- 4.1.8. **Potable Water Supply Ball Valves:** T-304 stainless steel
 Steam Supply Ball Valves: T-304 stainless steel
- 4.1.9. **Recirculation Header and Piping:** T-316L stainless steel
Interior Finish: 35Ra or better Electro-polished to 15 Ra finish 20Ra
Exterior Finish: 35Ra or better
- 4.1.10. **Sanitary valves:** T-316L stainless steel diaphragm valves
Interior Finish: 35Ra or better Electro-polished to 15 Ra finish
- 4.1.11. **Tri-Clamp Clamps:** T-304 stainless steel
- 4.1.12. **Fasteners:** T-304 stainless steel
- 4.2. **Unit Design:**
 The equipment is designed to be shipped and installed as a **single unit**. Some parts may be removed prior to shipping (i.e., pumps) to decrease the possibility of damages during shipping. The maximum crate size will be approximately _____" x _____" x _____" with an estimated weight of _____ lbs.
- Bolted and gasketed** construction allows the washer to be taken down prior to crating. There will be approximately _____ # separate pieces and the largest piece will be approximately _____" x _____" x _____" with an estimated weight of _____ lbs. A minimum clearance of _____" x _____" is necessary for access into the building. It is strongly recommended Girton Manufacturing Co., Inc. be contracted to re-assemble or supervise the re-assembly of the equipment due to the custom nature of the equipment.
- 4.3. All **internal corners** have a minimum 5/16" radius.
- 4.4. See enclosed **Girton's Welding Specification** for information on current in-house welding procedures.
- 4.5. All visible **welds** on the exterior of the washing compartment are thoroughly cleaned. All welds on the interior of the washing compartment are ground and polished.
- 4.6. The **cabinet interior** is constructed to permit free draining and designed not to retain any of the process solutions.
- 4.7. The **wash compartment** is sloped to drain into the pump reservoir through a stainless steel debris screen. The screen is easily removable without the use of tools.
- 4.8. The **washer tank capacity** is approximately 4-gallons of water, assuring effective cleaning and economy of operation. Level control is by means of a **stainless steel float switch, which is** tied into the washer control system.
- 4.9. All four sides and top are **insulated** with rigid foam and covered with a full jacket. This insulation package greatly reduces radiated heat loss from the washer making it more economical to operate and affords more comfort for the operators.
- 4.10. **Single door operation** the **self-supporting drop down door, when open**, works as a load table for rollout racks. The door is balanced for easy operation by gas-assisted cylinders.
- The **door** is double walled and insulated with rigid foam insulation. It is also baffled and gasketed against water leakage from the wash chamber. The door gaskets are closed cell silicone. The door has an 8" x 8" vapor-proof, heat-tempered glass **viewing window**. The window is sealed against water leakage by a silicone gasket. A **door safety switch** will be provided to stop the cycle and shut down the washer operation in the event that the door is opened during a cycle
- 4.11. The wash tank is provided with a **steam heating coil** controlled by the control system (adjustable) to maintain the wash/rinse solutions at a pre-set temperature. A line strainer is supplied on the steam supply connection as well as condensate traps, where necessary.
- The wash tank is provided with 15 KW **electric immersion heaters** controlled by the control system (adjustable) to maintain the wash/rinse solutions at a preset temperature.

- 4.12. **Pumps:**
- 4.12.1. **Recirculating wash/rinse pump** is a T-316 stainless steel horizontal centrifugal type unit, powered by a 2 Hp motor. It is capable of delivering 60-gallons per minute at 34' head pressure.
- 4.13. **Potable water supply ball valves** are threaded connections.
 Steam supply ball valves are threaded connections.
- 4.14. All **ancillary valves and equipment are positioned** on the washing machine top, rear and the side of the washer. Access to the serviceable items will be through removable panels located on the load end of the unit
- 4.15. **Recirculation Headers** consist of two rotating headers, employing properly spaced orifices these orifices direct the process solutions from the top, and bottom to assure complete and positive coverage. Upper header is permanent in washer, lower header is part of rack.
- 4.16. **Sanitary valves** have an **EPDM diaphragm** and tri-clamp ends
- 4.17. **Tri-clamp connection** use **EPDM gaskets** and are connected by means of heavy-duty clamps with wing nuts.
- 4.18. **Seals, gaskets, and bearings** are compatible with the temperatures and concentrations of cleaning agents to be used. Customer will supply information on chemicals to be used.
- 4.19. The **washer drains** by gravity. A pneumatically activated two-way ball valve directs the discharge to the drain.
- 4.20. **A compressed air system** is supplied with a filter regulator.
- 4.21. The washer is piped and wired for **single service connection** for each utility requirement.

5. CONTROLS AND OPERATION

- 5.1. The control system incorporates an **Allen Bradley Micrologix @PLC**, with Ethernet communication ability. The processor is aware of and controls all items on the washer. I/O cards are selected to match the control voltage. An isolated relay card is used to control high current draw items or items not operable at the control voltage. Analog cards are set to accept 4 - 20 mA inputs, unless otherwise noted.
- 5.2. The operator-machine consists of an **Allen Bradley Color Panelview Plus 600**, which incorporates a touch screen for operator control. This allows the user with proper password level to access all parameters of a wash recipe. All alarms are shown on the display, as well as announced audibly.
- 5.3. The washer is provided with the ability to use a printer to record operation reports. The customer should mount the printer close to the washer. Communication to the printer is RS232C so the maximum recommended distance from the washer is 50 ft. The report contains the following data: machine identification, operator, date and time, step name with time, temperature (min-max), etc.
- 5.4. **A typical treatment cycle** is defined as follows:
 Pre-Wash – Recirculated
 Wash – Recirculated
 Rinse – Recirculated
 Rinse – Recirculated
 Final Rinse--Recirculated
- 5.5. A total of **16 programs** can be stored in the PLC. Each program can be altered or developed from the OIT. Access to change or develop the programs is password protected.
- 5.6. Girton provides three levels of **password protection** to the control system:
Operator Level – access to selection of existing programs only
Maintenance Level – access to all maintenance screens
Engineering Level – access to all levels. Allows changes to be made to existing programs and new programs to be developed.
- 5.7. Girton's control system provides the ability to **alarm on abnormal conditions**. The washer has alarms based on each I/O point failure. This provides a comprehensive way of determining a device failure or process deviation. In general, all analog inputs to the system will have low and high alarm points settable by the customer. Also, all safety devices, such as door switches or emergency stop buttons, have alarms associated with them.

- 5.8. **Fused disconnect switch** is supplied and located in the main electrical enclosure to cut power to the entire unit. The system is designed so if the disconnect is in the "ON" position the electrical enclosure is not be able to be opened.
- 5.9. The washer is equipped with **Emergency Stop** switches located at critical points on the machine. All doors are equipped with limit switches wired directly to the output voltage. Opening any door will disconnect voltage from output cards thereby shutting down the system. These switches are also wired as inputs to the PLC so that an alarm may be generated. All services are equipped with fail-closed-valves.

6. DOCUMENTATION

- 6.1. **3 Hard copies and 1 electronic copy of Girton Documentation Package.** Validation requirements and considerations are playing an increasingly major role in the purchase of new equipment or systems. Validation requires documented evidence that the equipment or system will reliably perform in a manner consistent with the original design specifications. Generation of this documentation needs to be considered at the inception of the project and implemented throughout the design and manufacturing stages of the equipment. In most instances, the equipment vendor is the most qualified party to generate the majority of the required documentation.

The documentation provided by Girton Manufacturing Co., Inc. is designed to be a complete package including all data and checklists necessary to qualify the installation and operation of the equipment and/or system. All equipment built by Girton is completely factory assembled and tested. The documentation is used to perform Factory Acceptance Testing; witnessed and approved by the customer. All tests necessary for Installation and Operation Qualification of the equipment are performed on the equipment prior to its arrival on the job-site. Any modifications or additions required to qualify the equipment can be made at the factory prior to shipment. This index lists all documentation supplied by Girton Manufacturing Co., Inc.

1 DRAWINGS

DRAWINGS

Installation/General Arrangement

P&ID – Piping and Instrumentation Drawing

ELECTRICAL SCHEMATICS & PANEL DRAWINGS

ELECTRICAL SCHEMATICS - 3 Phase Wiring Diagrams, Control Wiring Diagrams, I/O Wiring Diagrams

PANEL LAYOUTS - PLC Panel Layout, Motor Starter Panel Layout

AIR PIPING SCHEMATICS

2 EQUIPMENT DATA

INSTRUMENT LIST

Tag numbers, manufacturer, model number, serial number, and description for all instruments installed on the washer.

MECHANICAL EQUIPMENT LIST

Component description, manufacturer, model number, and materials of construction.

CONTROL SYSTEM COMPONENT LIST

Tag numbers, manufacturer, model number, serial number, and description for all control system components installed on the washer.

EQUIPMENT LUBRICATION LIST

List of lubricants used to maintain the washer.

USER MANUAL

Instructions for operating the equipment including loading, unloading, control system operation, and safety precautions. Maintenance schedules and repair procedures for all equipment and instruments.

CALIBRATION AND CERTIFICATION

Calibration sheets, certifications and procedures for calibrating all critical instruments provided by Girton.

(SHORT TERM) PRICED SPARE PARTS LIST

PRICED SPARE PARTS LIST

Listing of replacement parts and their corresponding order numbers. Instructions on information required when ordering replacement parts.

COMPONENT CATALOG BROCHURES

Manufacturer's catalog information concerning installation, operation, and maintenance procedures for all purchased mechanical equipment and instruments.

CUSTOMER SERVICE POLICY

Tells about the warranty, damages, replacement parts, returned merchandise, field service, cancellation, and special equipment.

3 SOFTWARE DATA

QUALITY AND PROJECT PLAN

Defines the quality and project objectives for the washer and its automated control system.

FUNCTIONAL SPECIFICATION

Outlines functional requirements for the equipment.

HMI & PLC DESIGN SPECIFICATIONS

This document defines the hardware and software specifications for the washer and its component parts. The purpose of this document is to describe the complete operation of the automated process control system for the washer.

PROGRAMS ON CD

RS VIEW

Reports generated by the display software, which define screen elements and tag numbers corresponding to PLC addresses.

PLC RS LOGIX 500 PROJECT REPORT

Annotated listing of all code used to implement the software design.

4 FACTORY ACCEPTANCE TEST

- ABXXX FAT Instructions / Reference
- ABXXX Section 02 FAT Approval Drawing Review Test
- ABXXX Section 03 FAT Instrument Tests
- ABXXX Section 04 FAT Mechanical Equipment Tests
- ABXXX Section 05 FAT Electrical Tests
- ABXXX Section 06 FAT Utility Tests
- ABXXX Section 07 FAT Control System Hardware Tests
- ABXXX Section 08 FAT Control System Software Tests
- ABXXX Section 09 FAT Calibration Tests
- ABXXX Section 10 FAT HMI Tests
- ABXXX Section 11 FAT Operation Tests
- ABXXX Section 12 FAT Alarm Tests
- ABXXX Section 13 FAT Power Failure Tests
- ABXXX Section 14 FAT Summary Report Tests
- ABXXX Section 15 FAT Project Tests
- ABXXX FAT Signature Log
- ABXXX FAT Instrument Log
- ABXXX FAT Exception Log
- ABXXX FAT Test Progress Sheet
- ABXXX FAT Exception Form

5 PASSIVATION & PUNCHLIST REPORTS

- Passivation Procedure
- Passivation Report
- Completed Punchlist

VOLUME 3 OF 4

6 SITE ACCEPTANCE TEST

- ABXXX SAT Instructions / Reference

ABXXX Section 02 SAT Approval Drawing Review Test
ABXXX Section 03 SAT Instrument Tests
ABXXX Section 04 SAT Mechanical Equipment Tests
ABXXX Section 05 SAT Electrical Tests
ABXXX Section 06 SAT Utility Tests
ABXXX Section 07 SAT Control System Hardware Tests
ABXXX Section 08 SAT Control System Software Tests
ABXXX Section 09 SAT Calibration Tests
ABXXX Section 10 SAT HMI Tests
ABXXX Section 11 SAT Operation Tests
ABXXX Section 12 SAT Alarm Tests
ABXXX Section 13 SAT Power Failure Tests
ABXXX Section 14 SAT Summary Report Tests
ABXXX Section 15 FAT Project Tests
ABXXX SAT Signature Log
ABXXX SAT Instrument Log
ABXXX SAT Exception Log
ABXXX SAT Test Progress Sheet
ABXXX SAT Exception Form

7 WELDING

Procedure Qualification Record (PQR)
Weld Procedure Specifications (WPS)
Welding Procedure Qualifications (WPQ)
Weld Inspector Qualifications
Weld Logs and Weld Maps.

8 CERTIFICATIONS

Material Certifications sent with raw materials and some instruments ordered specifically for this project

Work Order Trace Report
Material Test Reports
Certificates of Conformance/Compliance

7. SERVICE REQUIREMENTS

- 7.1. **Electrical:** 3 phase, 60 cycle, 208 230 460 volt, _____ amperes.
- 7.2. **Hot Water:** 180°F. Recommended minimum rate of flow of 10 gallons per minute. 3/4" tri-clamp connection to the machine 16-gallon consumption/cycle.
- 7.3. **Purified Water** 180°F minimum flow rate 10 gpm at 30 PSI. 3/4" tri-clamp connection.
- 7.4. **Steam:** 40 to 80 PSI. 1/2" NPT connection to the machine (for most efficient operations, 60 PSI is recommended). 50-lb./hr. requirement.
- 7.5. **Condensate:** 3/4" NPT.
- 7.6. **Drain:** 1 1/2" NPT from the machine to the drain.
- 7.7. **Ventilation:** 4" diameter vent collar is provided for connection to ventilating system 50 CFM minimum removal required. Connection should be installed inside of vent collar to prevent leakage.
- 7.8. **Compressed Air:** 1/4" NPT connection 90-PSI minimum, 1 CFM.

8. WARRANTY

- 8.1. Girton Manufacturing Co., Inc. warrants equipment of original manufacture against defect in workmanship and material for a period of one year from date of shipment. Provided; however, the equipment has been operated under normal working conditions for such said equipment, that it has

been properly serviced and cared for, and that no adjustments have been made by unauthorized personnel that could adversely affect the operation or life of the equipment.

Girton Manufacturing Co., Inc. will replace or repair defective merchandise at its plant, FOB Millville, PA, if after inspection; the equipment or components that Girton manufactured are defective. Girton Manufacturing Co., Inc. extends to its customers on all purchased components parts, the warranty of the supplier of such said parts.

No expense, liability, or responsibility will be assumed by Girton for repairs outside Girton's factory, without written authority from Girton Manufacturing Co., Inc.

The foregoing warranty excludes all other warranties, guaranties, and/or representations; whether expressed, implies, or oral, INCLUDING, BUT NOT LIMITED TO, ALL CONDITIONS AND EXCLUSIONS OF IMPLIED WARRANTY OF MERCHANTABILITY AND OR FITNESS FOR THE PURPOSE, and the warrantor's liability for any direct damage arising from a legally proven breach of the warranty hereby extended is limited to the customer's invoice cost of the goods warranted.

- 8.2. DISCLAIMER OF CONSEQUENTIAL DAMAGES LIABILITY - Girton Manufacturing Co., Inc. shall not be liable for consequential damages of any kind, including incidental labor or other costs.

9. CANCELLATION

- 9.1. Any order on which work had been started may be cancelled only by consent of Girton Manufacturing Co., Inc. and by agreement on the part of the purchaser to cover whatever cost has been incurred, if any, to the date of the cancellation, including engineering, administrative, material purchases, labor, and overhead expended.

10. CUSTOMER TO WITNESS PRELIMINARY FACTORY ACCEPTANCE TEST (FAT)

10.1. General Description:

A factory acceptance test (FAT) will be performed at Girton's facility in Millville, PA prior to shipment. The customer will provide written permission allowing delivery of the washing system once the FAT has been successfully completed.

Factory test will meet the requirements outlined in the FAT protocol provided by Girton. The FAT protocols will be sent to the customer before commencement of the scheduled FAT. These FAT protocols are to be reviewed, approved and returned to Girton prior to the scheduled FAT date. Girton will note any changes required and notify the customer should this have an impact on scheduled FAT date.

Samples of all the items that will be cleaned along with the cleaning chemical the customer plans on using will need to be sent to Girton prior to the FAT. These items will be returned, with the washing system, once the FAT has been successfully completed.

Note: A MSDS must accompany the shipment of any chemical.

If scheduling allows, Girton will perform and document the Pre-FAT prior to the customer's arrival. The results of this testing will be available for the customer to review at time of customer's FAT.

Girton highly recommends the customer witness the FAT to inspect design, adherence to the specification and construction on the supplied washing system. The customer has the right to add additional tests at the time of the approval of the FAT protocols. Any additional tests will need to be approved by Girton. If additional costs are incurred, a change order will need to be issued by the customer.

Included in the contract price of the equipment are 3 days for the customer to execute the FAT. A Girton instrument technician will be available to assist the customer during the FAT. If additional days are required please reference Fig. 1 for the additional charges.

Girton allows equipment check out by 3rd party inspection services. In addition to the FAT charges a daily fee is charged for each day the inspector is on site at Girton Manufacturing Co., Inc. Reference Fig.1 for the additional charges.

10.2. Standard FAT protocols will be provided for the following:

- General Arrangement and P&ID review
- Instrument checks

- Mechanical Equipment checks
- Wiring Continuity Check
- Utility Connections
- Control system hardware verification
- Control System Software Test
- Calibration and Scaling Test
- Operator Interface function and screen layout Test
- Control System I/O Test
- Equipment Alarms Test
- Power Failure Test

Operation of the washing system will be at ambient temperature during the checkout phases of protocols. The washing system will operate one heated cycle to complete the FAT.

For safety reasons only Girton personnel will operate the equipment. Non-Girton personnel are required to comply with Girton safety procedures. A copy of these procedures is available upon request.

10.3. **Utilities available for use during Girton FAT:**

- ❖ Electrical: 3 Phase 60 cycle 208/230/460/500/other volt
- ❖ Hot Water: approx. 140° F
- ❖ Cold Water: ambient
- ❖ Industrial compressed air: 100 psi
- ❖ 1 mega ohm Purified Water: approx. 140° F
- ❖ Steam: approx. 80 psi

10.4. **Additional FAT Charges (Fig. 1)**

Item	Cost
Additional days for FAT includes Girton Instrument Tech.	\$1,250.00/day
Storage*	\$395.00/day
Disconnecting and Connecting	\$750.00/each
3rd Party Inspection	\$1,175.00/day
Girton Programmer	100.00/hr.
Girton QA Personnel	\$100.00/hr
Girton Instrument Tech.	\$60.00/hr

*Storage fees are incurred in the following situations:

- Delayed FAT -The customer cannot attend within the scheduled time frame.
 - Girton will perform the Pre-FAT, disconnect the equipment from the utilities and place it into short-term storage. Once the customer has confirmed their FAT dates the equipment will be returned to the testing area and reconnected to the utilities. Cost for disconnecting and connecting to utilities are listed in Fig. 1.
- Delivery Delay-The FAT has been successfully completed and the customer cannot accept delivery.

11. DOCUMENTS

11.1. ___ # sets of **Approval Documents** will be provided to the Customer in ___ days weeks after receipt of order. Production work will not be initiated until these drawings are returned to Girton Manufacturing Co., Inc. with the appropriate signatures of the customer.

12. INSTALLATION

- 12.1. Installation will be **done by others**.

13. TERMS AND CONDITIONS

- 13.1. Payment Terms:
25 % With Order and 75 % Due 30 Days After Shipment,
1-1/2% per month finance charge will be added thereafter.
- Payment Terms:
25% Down
65% Upon shipment
10% Upon successful start-up, not to exceed 60 days from shipment.
- A pre-approved Progressive Payment Terms, *which must be spelled out here:* _____
- 13.2. The 6% PA sales tax will be assessed on all sales. If you believe the products covered by this proposal are exempt from this tax, please send to Girton Manufacturing Co., Inc. your PA sales tax exemption certificate.

14. SHIPPING

- 14.1. Freight terms:
 Collect
 Prepaid by customer and add to Invoice
 Third Party Billing
- 14.2. Shipment will be provided by transportation arranged by Girton Manufacturing Co., Inc.
 customer.
- 14.3. Shipment from Millville, PA ___ to ___ weeks, after receipt of signed Documents by Girton Manufacturing Co., Inc.

15. TOTAL COST PER THIS SPECIFICATION, CONSULT FACTORY

16. OPTIONS

- 16.1. The Human Machine Interface (HMI), mounted on the washer, consists of a PLC based display, which will be programmed using RSView SE software, which incorporates a touch screen for operator control and monitoring. This allows the user with proper password level to access all parameters of a wash recipe. All alarms are shown on the display, as well as announced audibly. Use of this system complies with CFR21 Part 11.
- 16.2. **Pass through operation** is accomplished with two (2) **self-supporting drop down doors**. When the doors are open they work as load tables with rollout racks. Each door is balanced for easy operation by gas-assisted cylinders.
- Each door is double walled and insulated with rigid foam insulation. The doors are baffled and gasketed against water leakage from the wash chamber. Door gaskets are closed cell silicone. The doors are provided with a 16" x 18" vapor-proof heat tempered glass as a viewing window. The window is sealed against water leakage by means of a silicone gasket. A **door safety switch** is provided for each door. The switch shall stop the cycle and shut down the washer operation in the event that either door is opened.
- 16.3. **Door interlocks** prevent the load and unload door from being opened simultaneously. This system consists of two pneumatic air cylinders, two control valves all controlled by the washer controller.
- Operation shall be as follows:
Load door open - unload door is locked.
Unload door open - load door is locked.
Washer operating or idle - both doors are unlocked.
- 16.4. Front of washer is designed with **facia and concealment panels** providing a flush appearance when installed through one wall. Height of facia will exceed height of any permanently mounted component of washer system located on top of washer, except where it can be removed for installation.

- 16.5. **Service-side shroud** is provided to enclose the service side of the washer. Shroud is easily removable for service access.
- 16.6. **T-316L construction** on all wetted surfaces.
- 16.7. **Interior finish** to be a 35Ra or better finish.
- 16.8. **Drying** - The tank is automatically drained prior to the start of the drying cycle. The dryer consists of a recirculated hot air system utilizing steam coils electric heating elements and a high volume blower to circulate hot air over the items to be dried. A small amount of room air is drawn into the system to aid in maintaining proper humidity levels for efficient drying. The controller controls the drying cycle and temperature. This option adds 6" to the height of the unit.
- 16.8.1. Stainless steel air stream of T-304 T-316L. Blower is fabricated of T-304 T-316L stainless steel. A HEPA filter is provided on discharge of blower.
- 16.9. A **light fixture** mounted on the exterior of the unit illuminates the wash chamber during operation.
- 16.10. The discharge pressure of the main circulation pump is monitored using a **sanitary pressure transmitter**. This pressure is recorded and alarmed by the control. The diaphragm of the sensor is attached in the wash pump discharge line using a tri-clamp connection. Girton's standard range for measuring pump pressure is 0 to 100 psi. Girton's preferred vendor is Rosemount for the instrument.
- 16.11. All **compressed air lines** are T-304 stainless steel with Swagelok compression split ferrule type fittings.
- 16.12. A **sample port** in the recirculation sump allows sampling of the water from the face of the washer. The sample port is attach via tri-clamp with connecting piping to have sufficient pitch in order to drain back into the washer recirculation tank, thus eliminating the possibility of dead legs.
- 16.13. A **drain tempering system** cools the process wash and rinse solutions from 180° F to 140° F prior to entering the customer's drain. This system consists of a temperature control with a probe located in drain line for on-off control of cold water supply valve.
- 16.14. The **conductivity** of any wash solution where a reagent is added is monitored, recorded and, if needed, alarmed by the control. A sensor is attached either in the wash pump discharge or directly into the sump. Both are inserted into a sanitary tri-clamp connection. Girton's standard range for measuring wash solution conductivity is 0 to 100 milli-siemens.
- 16.15. The **conductivity** of the final rinse with the customer's designated water will be monitored, recorded and, if needed, alarmed by the control. The sensor is attached in or near the drain line with a sanitary tri-clamp connection. Girton's standard range for measuring final rinse conductivity is 0 to 100 micro-siemens.
- 16.16. **Girton neutralization system** will be provided for the purpose of neutralizing the wash solution before going to drain. This system will include a **chemical pump** to inject the neutralizing solution and the necessary divert valves to stop the flow of water from going to the headers and direct it back to the washer sump to mix the neutralizing solution.
- 16.17. **Girton neutralization system with pH monitor** will be provided for the purpose of neutralizing the wash solution before going to drain. This system will include a **chemical pump** to inject the neutralizing solution and the necessary divert valves to stop the flow of water from going to the headers and direct it back to the washer sump to mix the neutralizing solution. The pH sensor will signal the washer PLC when the solution had reached the desired level so the drain valve can open.
- 16.18. **Automatic detergent dispenser** is provided with the control system. One (1) peristaltic pump with 120VAC motors is used to charge the wash solution with the desired reagent. The customer sets the amount of time that each dispenser will run for the wash cycle.
- 16.19. For each reagent reservoir, Girton supplies a **level monitor**. The monitor will consist of an ultrasonic sensor that will switch a PLC input when the reagent reaches the specified level. The control can then either trigger an alarm or a status message based on the input. The sensor has threads allowing it to be mounted into the lid of the customer's detergent reservoir.
- 16.20. A **remote mounted Epson LX300 printer** will be provided so that a printed record of each cycle can be obtained.
- 16.21. The washer is specified to be in a **Class I Division 2 Group D area**. All wiring, conduit, instruments, and other devices conform to the NEC and NFPA regulations for the class and division of the washer. If required, purged enclosures will be provided as well as explosion resistant conduit.

- 16.22. All **conduit** on the machine are PVC coated rigid. Fittings and conduits are PVC coated as well. Liquid tight flexible conduit is used to connect the washer's devices. Lengths of flexible conduit do not exceed 3 feet. All marks on conduit are painted with PVC paint. All conduit installation meets the current NEC requirements.
- 16.23. Each motor under control have a locally mounted **HAND-OFF-AUTO** switch and a "Run" light. In HAND position, the motor runs; in OFF position, the motor stops; in AUTO position, the motor is under PLC control.
- 16.24. An **exhaust fan**, wired and mounted on machine, including manual damper, is provided. The fan will exhaust 300 CFM to the ventilating system or to the outside. A 6" diameter vent collar is also provided. The connection is installed inside of vent collar to prevent leakage.
- 16.24.1. T-304 T-316L stainless steel air-stream.
- 16.25. An **automatic vent damper** is interwired with washer control system. The damper travel is adjustable and is set once unit is installed in the customer's facility.
- 16.26. The wash tank is provided with **electric immersion heaters** controlled by the control system (adjustable) to maintain the wash/rinse solutions at a preset temperature. Total KW required, for electric heating only, equal 54 KW.
- 16.27. A **pass-through heat exchanger** raises the incoming potable water temperature from 140°F to 180°F. This option is required when fast cycle times are required and ample hot water is not available from the facility supply.
- 16.28. **Spindle headers** fabricated of stainless steel is designed to properly support glassware, plastic ware, drums, carboys, etc., over individual spray nozzles. The header can be loaded and unloaded on the drop-down door and rolled into the washer.

Possible rack configurations:

- Miscellaneous glassware spindle rack
- 100 position spindle rack
- 12 position spindle rack
- 9 position spindle rack
- 3 position spindle rack

Note: A sample of each glassware is required to assure spindle header design.

- 16.29. A roll-in T-304 stainless steel **immersion parts cart** is provided. This is a combination agitating bath and spray cleaning system. The parts are immersed in the cleaning solution and the recirculation pump creates the agitating action within the immersion parts rack. The rack constantly overflows the cleaning solution and returns it to the recirculation sump. This process is run using a separate program.
- 16.30. A **transfer table** allows the various headers to be removed from the washer for transportation, loading/unloading, or storage. The table is fabricated of stainless steel with a centering device to line up with the washer door and a device to lock the rack to the table. The table will run on four swivel casters.
- 16.31. **Additional copies of our Documentation Package** (reference item # _____ of this specification) may be purchased.
- 16.32. **Optional Documentation:**
- 16.32.1. Surface Finish Map and Certificate of Compliance
- 16.32.2. Slope Map of Process Contact Tubing and Certificate of Compliance
- 16.32.3. Video Weld Logs
- 16.32.4. Sound Level Certificate of Conformance
- 16.33. **Supervision of installation (YSOFI)** – Girton Manufacturing Co, Inc. will provide ONE Qualified Technician for ____ (# of days) contiguous* on-site days to Supervise and Direct Customer Personnel, Contractors or Subcontractors in all phases of Installation. This includes oversight of Uncrating and Moving the Equipment into a prepared⁽¹⁾ Wash Room, Leveling and Reassembly, Utility⁽²⁾ and Additional Support Systems⁽³⁾ Connections. Supervision of Unloading the Shipping Truck will be performed *only if* delivery occurs during the scheduled timeframe.

Supervision of Installation (Sofl) does **not** include Sub-Contracting, Equipment or Tools or Tool Rental, Dumpsters and/or Trash Disposal, Multiple Trips from our Factory (except at our discretion and as deemed necessary by our Technical Service Manager), Additional Site Preparation, Materials for Floor Protection, Integration Materials or Fabrication (other than Modular Walls, Fascia Panels, and items purchased from Girton Mfg. as an option), Equipment Start Up, Training of Personnel or Assisting with SAT or Validation Documentation.

The Customer will be responsible for all facets of installation not specifically included above. Equipment Start Up, Training of Personnel, Assisting with SAT or Validation Documentation may be purchased from Girton separately.

A Field Report will be submitted to the Customer within one week of completion of the installation.

Supervision of Installation is a quoted option and valid as part of the original equipment order. Service ordered after the original equipment order date will require a requote. Travel expenses are included in the first day billing. Additional contiguous days may be purchased for a flat fee of \$____.00 per day, but should be purchased prior to the first on-site day, if possible. This information is based on non-union labor. Special provisions and prices apply when union labor and/or prevailing wages are required. Contact your Sales Rep for further details.

- 16.34. **Set-in-place Installation (YSIP)** - Girton Manufacturing Co, Inc. will provide Qualified Technicians for ____ (# of days) contiguous* on-site days to Unload and Uncrate, Move the equipment to a prepared⁽¹⁾ location, Reassemble and Level the Equipment. Girton Manufacturing Co, Inc. will provide all Personnel, Material, Tools and Equipment to perform the task, including Fork Trucks, Dumpsters, Welders, Hand Tools, Floor Protection and Trash Elimination.

Set-In-Place Installation (SIP) does **not** include Utility⁽²⁾ Connections, Connection of Additional Support Systems⁽³⁾, Multiple Trips from our Factory (except at our discretion and as deemed necessary by our Technical Service Manager), Additional Site Preparation, Integration Materials or Fabrication (other than Modular Walls, Fascia Panels, etc., purchased from Girton Mfg. as an option), Equipment Start Up, Training of Personnel or Assisting with SAT or Validation Documentation.

The Customer will be responsible for all facets of installation not specifically included above. Equipment Start Up, Training of Personnel, Assisting with SAT or Validation Documentation may be purchased from Girton separately.

A Field Report will be submitted to the Customer within one week of completion of the installation.

Set-In-Place Installation is a quoted option and valid as part of the original equipment order. Service ordered after the original equipment order date will require a requote. Travel expenses are included in the first day billing. Additional contiguous days may be purchased for a flat fee of \$____.00 per 8 Hr. man-day, but should be purchased prior to the first on-site day, if possible.

This information is based on non-union labor. Special provisions and prices apply when union labor and/or prevailing wages are required. Contact your Sales Rep for further details.

- 16.35. **Complete Installation (YINSTALL)** - Girton Manufacturing Co, Inc. will provide Qualified Technicians for ____ (# of days) contiguous* on-site days to Unload, Uncrate, Move the equipment to a prepared⁽¹⁾ location, Reassemble, Level the Equipment and Connect Utilities⁽²⁾ to **existing stubs** within 6' of the machine. Girton Manufacturing Co, Inc. will provide all Personnel, Material, Tools and Equipment to perform the task, including Fork Trucks, Dumpsters, Welders, Hand Tools, Floor Protection and Trash Elimination. Test and Demonstration (see below) is part of this option. If this cannot be completed contiguously (due to unavailable utilities, Customer personnel availability, etc.), a return trip must be scheduled and additional travel expenses will apply.

Complete Installation (CI) does **not** include Multiple Trips from our Factory (except at our discretion and as deemed necessary by our Manager), Additional Site Preparation, Connection of Additional Support Systems⁽³⁾, Integration Materials or Fabrication (other than Modular Walls, Fascia Panels, etc., purchased from Girton Mfg. as an option), Equipment Start Up, Training of Personnel or Assisting with SAT or Validation Documentation.

The Customer will be responsible for all facets of installation not specifically included above. Equipment Start Up, Training of Personnel, Assisting with SAT or Validation Documentation may be purchased from Girton separately.

A Field Report will be submitted to the Customer within one week of completion of the installation.

Complete Installation is a quoted option and valid as part of the original equipment order. Service ordered after the original equipment order date will require a requote. Travel expenses are included

in the first day billing. Additional contiguous days may be purchased for a flat fee of \$____.00 per 8 Hr. man-day, but should be purchased prior to the first on-site day, if possible.

This information is based on non-union labor. Special provisions and prices apply when union labor and/or prevailing wages are required. Contact your Sales Rep for further details.

- 16.36. **Test and Demonstration (YTD)** - Girton Manufacturing Co, Inc. will provide ONE Qualified Technician for ____ (# of days) contiguous* on-site days to perform Start Up Testing, such as verifying utility connections and capacities, electrical supply voltage and amperage, motor rotations, completeness of assembly, missing components, etc., on fully installed⁽⁴⁾ equipment. The Technician will make normal *equipment* adjustments and test operation against factory standards. Upon completion of satisfactory testing, the Technician will demonstrate all phases of the use and operation of the equipment to any interested parties, provided sufficient time is allotted. We recommend that three to four hours be dedicated for effective demonstration. We highly recommend that at least one User of each level of access (Operator, Maintenance, Supervisor/Engineering, Administrative) be present for the demonstration. *Demonstration must not be confused with training; it is NOT a substitute for a complete and formal training session*, 'Demonstration' is informal, with the Technician covering the highlights of the equipment and operation and hazard awareness, and answering questions from interested parties. No handout sheets or post-training testing is given.

Test and Demonstration (T&D) does **not** include mechanical reassembly or completion of wiring or pneumatics (on-skid or otherwise), any function that is normally part of the three Installation options described above, Multiple Trips from our Factory (except at our discretion and as deemed necessary by our Technical Service Manager), Additional Site Preparation, or Assisting with SAT or Validation Documentation.

The Customer will be responsible for all facets of installation not specifically included above. Supervision of Installation, Set in Place Installation, Complete Installation, Training of Personnel, Assisting with SAT or Validation Documentation may be purchased from Girton separately.

A Field Report and a copy of an Attendance Record for the demonstration will be submitted to the Customer within one week from the end of the visit.

Test and Demonstration is a quoted option and valid as part of the original equipment order. Service ordered after the original equipment order date will require a requote. Travel expenses are included in the first day billing. Additional contiguous days may be purchased for a flat fee of \$____.00 per 8 Hr. man-day, but should be purchased prior to the first on-site day, if possible.

This information is based on non-union labor. Special provisions and prices apply when union labor and/or prevailing wages are required. Contact your Sales Rep for further details.

- 16.37. **Start Up (YSTART)** - Girton Manufacturing Co, Inc. will provide ONE Qualified Technician for ____ (# of days) contiguous* on-site days to perform Start Up Testing, such as verifying utility connections and capacities, electrical supply voltage and amperage, motor rotations, completeness of assembly, missing components, etc., on fully installed⁽⁴⁾ equipment. The Technician will make normal *equipment* adjustments and test operation against factory standards. Start Up does **not** include mechanical reassembly or completion of wiring or pneumatics (on-skid or otherwise), any function that is normally part of the three Installation options described above, Multiple Trips from our Factory (except at our discretion and as deemed necessary by our Technical Service Manager), Additional Site Preparation, or Assisting with SAT or Validation Documentation.

The Customer will be responsible for all facets of installation not specifically included above. Supervision of Installation, Set in Place Installation, Complete Installation, Training of Personnel, Assisting with SAT or Validation Documentation may be purchased from Girton separately.

A Field Report will be submitted to the Customer within one week from the end of the visit.

Start Up is a quoted option and valid as part of the original equipment order. Service ordered after the original equipment order date will require a requote. Travel expenses are included in the first day billing. Additional contiguous days may be purchased for a flat fee of \$____.00 per 8 Hr. man-day, but should be purchased prior to the first on-site day, if possible. This information is based on non-union labor. Special provisions and prices apply when union labor and/or prevailing wages are required. Contact your Sales Rep for further details.

- 16.38. **Training (YTR)** - Girton Manufacturing Co, Inc. will provide ONE Qualified Technician for ____ (# of days) contiguous* on-site days to formally and thoroughly provide in-depth training to Operators, Maintenance Technicians, Engineering and Administrative Level Personnel. Our Technician will

provide a combination of classroom and hands-on field training. A 'Question and Answer' period is encouraged.

16.38.1. **Topics covered are:**

Hazard Awareness,
Alarms and the causes of and responses to them,
Routine Operation,
Routine Maintenance and Trouble Shooting,
Set Up, Management and Modification of Recipes (Cycles),
User Management (Administration).

16.38.2. **Training (TRN)** covers the full range of access and use:

16.38.2.1. **'Operator'** level training covers the daily operation and maintenance, and is the shortest and most basic training.

16.38.2.2. **'Maintenance'** level training includes full Operator training and adds the extensive maintenance diagnostic capabilities available through the HMI, and PM requirements.

16.38.2.3. **'Engineering'** level training will include condensed Operator and Maintenance coverage and adds in-depth Recipe (Cycle) Generation and Management and Recipe and Alarm Set Points. Engineering training is typically restricted to those individuals responsible for control of validated operation.

16.38.2.4. **'Administrator'** level training will have condensed coverage for all levels of use, but will focus primarily on User Administration and Security. At this level, Users Names and Passwords are assigned and Levels of Access Controlled.

Whenever possible, a computer presentation will be shown and pertinent hand out sheets will be distributed. An Attendance Roster and post-training Retention Test will be given and copies will be provided to the Customer.

Training is a quoted option and valid as part of the original equipment order. Service ordered after the original equipment order date will require a requote. Travel expenses are included in the first day billing. Additional contiguous days may be purchased for a flat fee of \$_____.00 per day, but should be purchased prior to the first on-site day, if possible. This information is based on non-union labor. Special provisions and prices apply when union labor and/or prevailing wages are required. Contact your Sales Rep for further details.

16.39. **Site Acceptance Testing Assistance (YSAT)** - Girton Manufacturing Co, Inc. will provide ONE Qualified Technician for ____ (# of days) contiguous* on-site days to assist the Customer's Validation Group(s) with IQ/OQ of fully installed⁽⁴⁾ and running equipment. Girton Mfg. will provide an SAT Template based on the factory test documents and appropriate programming software and test instruments necessary to duplicate the factory tests. Girton Technicians will assist the Customer by providing clarification of test procedures and test results, and through our experience with the PLC and HMI Programming. Sample SAT documents are typically submitted to the Customer for early review. Machine specific documents shall be submitted to the Customer a minimum of two weeks prior to SAT.

Girton Technicians will *not* be responsible for completing partial installations, test document revisions or test completion.

A Field Report will be submitted to the Customer within one week of completion of the SAT.

Site Acceptance Test is a quoted option and valid as part of the original equipment order. Service ordered after the original equipment order date will require a requote. Travel expenses are included in the first day billing. Additional contiguous days may be purchased for a flat fee of \$_____.00 per day, but should be purchased prior to the first on-site day, if possible. This information is based on non-union labor. Special provisions and prices apply when union labor and/or prevailing wages are required. Contact your Sales Rep for further details.

16.40. **Notes:**

16.40.1. ⁽¹⁾ "Prepared" site is defined as one at which the building is enclosed, the floor and floor coatings are complete and where Girton personnel can work reasonably unhindered. Electricity (for tools) *must* be available. It is preferred, but not mandatory, that utilities⁽²⁾ are complete and available.

- 16.40.2. ⁽²⁾ “Utilities” are defined as Potable Water (Hot and/or Cold), Steam, Condensate, Ventilation, Electrical, Compressed and/or Instrument Air, and Drains. “Utilities” does *not* include Purified (DI, WRO, WFI, etc.) water sources that require high-purity pipe welding, remote Detergent systems or controls, Chiller/Glycol system piping, Facility Control or Data Systems, networked or otherwise.
- 16.40.3. ⁽³⁾ “Additional Support Systems” are defined as Purified Water (DI, WRO, WFI, etc.), Chiller systems, Detergent Systems, Combustible Liquids or Gas, and Breathing Air. Connection of Additional Support Systems is *a/ways* the responsibility of the Purchaser.
- 16.40.4. ⁽⁴⁾ “Fully Installed” is defined as the equipment being in-place and leveled, and connected to all utilities and additional support systems. Integration with building fabric is not required.
- * Excluding Saturdays, Sundays and/or Holidays, unless prearranged.